

# Calibration Update

August 2017

## Perten AM5200-A system update instructions August 2017 implementation

### FORWARD

This instruction is a step by step direction for updating the AM5200-A moisture meter to the current Calibration Update for 08/01/2017.

**NOTE: If the unit does not have UI Software Version of 20160701.02, call (217) 585-9440 for further instructions.**

1. PROCEDURE.....	2
2. QUESTIONS .....	4

The U.S. Department of Agriculture (USDA) prohibits discrimination in its programs on the basis of race, color, national origin, sex, religion, age, disability, political beliefs, and marital or familial status. (Not all prohibited bases apply to all programs.) Persons with disabilities who require alternate means for communication of program information (Braille, large print, audiotape, etc.) should contact USDA's TARGET Center at (202) 720-2600 (voice and TDD).

To file a complaint, write to the USDA, Office of Civil Rights, Room 326-W, 1400 Independence Avenue, SW, Washington, DC 20250-9410, or call (202) 720-5964 (voice and TDD). USDA is an equal employment opportunity employer.

# 1. PROCEDURE


- a) Plug a USB flash drive into your computer
  - 1) Make sure this USB flash drive does not have a folder called 'Perten' on it currently.
  - 2) If there is a folder called 'Perten', delete or rename the folder before continuing.
- b) Go to [www.gipsa.usda.gov/fgis/moisture.aspx](http://www.gipsa.usda.gov/fgis/moisture.aspx) on your web browser
  - 1) Under the 'Official Moisture Calibrations' heading, right click the link where it says: 'Download all official moisture calibration files for Perten AM 5200-A'




- 2) Select 'Save Link as...' or 'Save Target as...'
- 3) When it asks for a location, select the USB flash drive you have plugged in.
- 4) Once the download is finished, on your computer, go to your USB stick and right click on the perten.zip file and Extract All.
- 5) Example Path:




- 6) In this 'Perten.zip' Press 'Extract all files'
- 7) When the next window pops up, press extract.

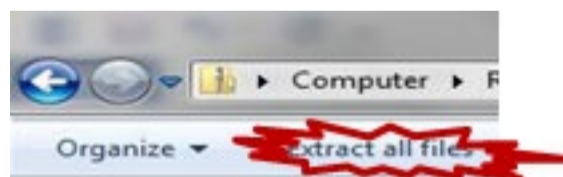

- c) Delete the perten.zip file from the USB flash drive.
- d) Turn on the power switch of the AM5200-A if it is not already operating. Connect the USB drive to either of the two ports on the back of the AM5200-A.

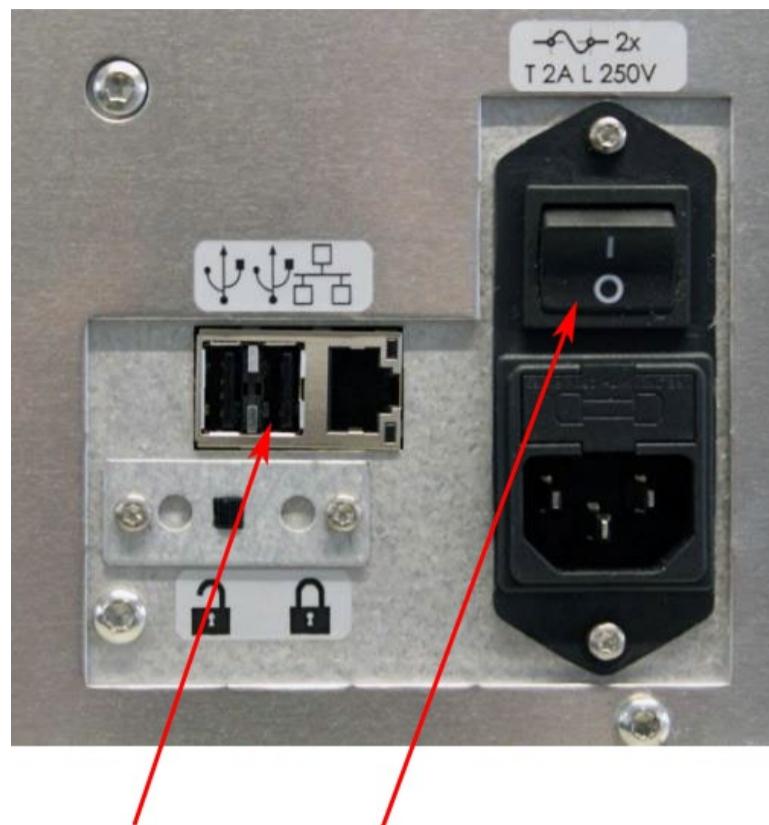


- e) Before installing new calibrations, a “restore point” should be set, which provides a backup in case the update process is interrupted. (Go to instrument.)
  - 1) Set access right to “administrator” on the AM5200-A (Menu - General settings - Login). Touch the word “default” to get an on-screen keyboard. Your administrator password is **142857** (unless you have changed it). Screen will show “Successfully logged in as Admin user”. Press “close” button.

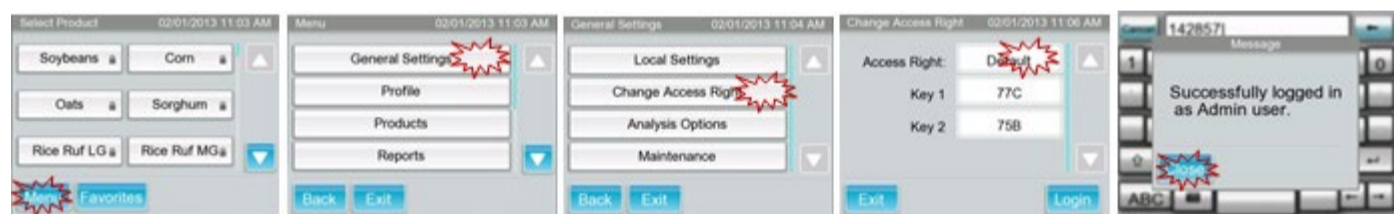

- 2) Select (Menu - General settings - Maintenance - System recovery - Set a restore point). The screen will show a list of system files being archived. When this is complete, the unit will restart.




- f) Reset access right to “administrator” on the AM5200-A (see step e1 for step-by-step instruction).
- g) Import the new settings (Menu - down-arrow – Import/export - Import). It will take some time to process the update file (up to 2 minutes). When the process is done, the message “Imported successfully. Please reboot the system” will appear. (If this message does not appear, remove the USB drive and start the process over from step d).

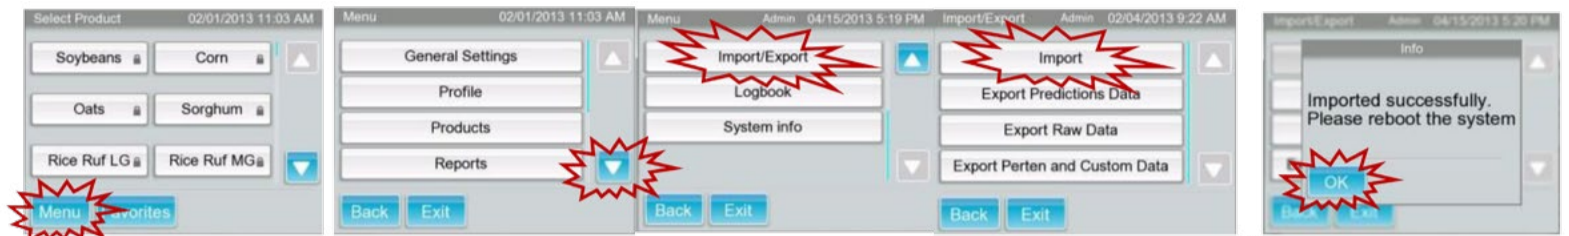

- h) Remove the USB drive, turn off the power switch for a few seconds, and then turn power on again.
- i) Confirm update: ( Menu / down arrow / System info / down arrow )button.



View the next page of system info (down-arrow again) to check Calibration Version 08-01-2017:

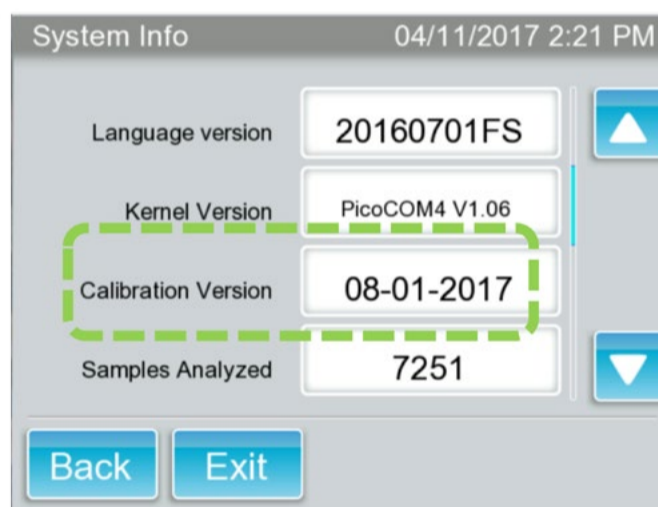

## 2. QUESTIONS

If you encounter any problems with this procedure, free phone assistance is available through Perten Instruments, 7 am to 6 pm Central time, Monday – Friday at (217) 585-9440.